

SARS-CoV-2 and handling of Dräger Anesthesia Workstations

February 20, 2020

Dear Sir or Madam,

The following information and recommendations are targeted for Anesthesia Workstations from Dräger that were used on patients infected or highly suspected to be infected with the novel coronavirus (SARS-CoV-2).

Background:

Coronaviruses (CoV) are a large family of enveloped viruses that cause illness ranging from the common cold to more severe diseases such as Middle East Respiratory Syndrome (MERS-CoV) and Severe Acute Respiratory Syndrome (SARS-CoV). The novel coronavirus (SARS-CoV-2) is a new strain that has not been previously identified in humans.

Coronaviruses are transmitted between animals and humans (zoonotic transmission). The possibility of transmission among humans especially of SARS-CoV-2 is now confirmed, but the extent of human-to-human transmission is still not clear.

The novel coronavirus (SARS-CoV-2) belongs to the category of enveloped viruses that in principle can be removed with disinfectants with limited virucidal effectiveness. However, for a higher safety level it is also possible to use locally registered hospital disinfectant with a label claim for a non-enveloped virus (e.g. norovirus, rotavirus, adenovirus, and poliovirus). Further information you can find on the following websites and further national organization websites:

- <https://www.who.int/emergencies/diseases/novel-coronavirus-2019>
- <https://www.cdc.gov/coronavirus/2019-ncov/index.html>
- <https://www.ecdc.europa.eu/en/novel-coronavirus-china>
- <https://www.rki.de/covid-19>

Drägerwerk AG & Co. KGaA
Moislinger Allee 53-55
23558 Lübeck, Germany
Postal address:
23542 Lübeck, Germany
Tel +49 451 882-0
Fax +49 451 882-2080
info@draeger.com
www.draeger.com
VAT no. DE135082211

Bank details:
Commerzbank AG, Lübeck
IBAN: DE95 2304 0022 0014 6795 00
Swift-Code: COBA DE FF 230
Sparkasse zu Lübeck
IBAN: DE15 2305 0101 0001 0711 17
Swift-Code: NOLADE21SPL

Registered office: Lübeck
Commercial register:
Local court Lübeck HRB 7903 HL
General partner: Drägerwerk Verwaltungs AG
Registered office: Lübeck
Commercial register:
Local court Lübeck HRB 7395 HL

Chairman of the Supervisory Board
for Drägerwerk AG & Co. KGaA
and Drägerwerk Verwaltungs AG:
Stefan Lauer
Executive Board:
Stefan Dräger (chairman)
Rainer Klug
Gert-Hartwig Lescow
Dr. Reiner Piske
Anton Schrofner

System setup recommendations for confirmed or highly suspected SARS-CoV-2-patients:

A. Essential measures

A1 Anaesthesia device:

- Use of a **mechanical breathing system filter** (BSF) such as MP01790 SafeStar 55 (adults only) at patient side (between tracheal tube and y-piece of the breathing circuit (hoses)). **Caution:** The gas sample line of the anesthesia device must be connected on the device side of the BSF in order to avoid contamination of the gas measurement unit and consequently the entire anesthesia device (see figure 1).

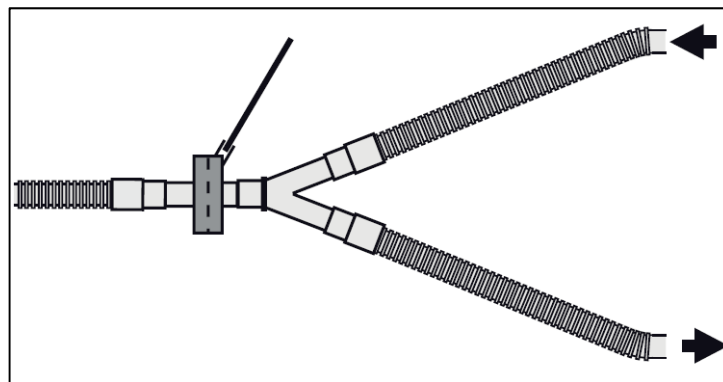


Figure 1

- Deploy **disposable breathing circuit** (hoses) only. For types and part numbers please see Dräger Accessory Catalogue.

A2 Endotracheal suctioning device:

- The VarioSafe® disposable filter system (MP00555) has to be used to reliably protect the suctioning device and the patient environment against contamination.
- We recommend to use Dräger Vacusmart Gel inserts for the suction canister.

A3 Monitoring accessories:

Disposable Monitoring accessories should be used and disposed after each patient.

- Disposable ECG leads
- Disposable SpO2 sensors
- Disposable NiBP cuffs
- Disposable temperature probes

For types and part numbers please see the Dräger Accessory Catalogue.

B. Optional measures (recommendation for a higher safety level)

An **additional Breathing System Filter (BSF)** at the expiratory port of the breathing system such as MP01785 SafeStar 80/ MP01795 SafeStar 60A/ MP01790 SafeStar 55 (between breathing hose set and expiratory port of the device) is strongly recommended because of contamination risk of the breathing system during daily disconnection and replacement of the BSF at patient side

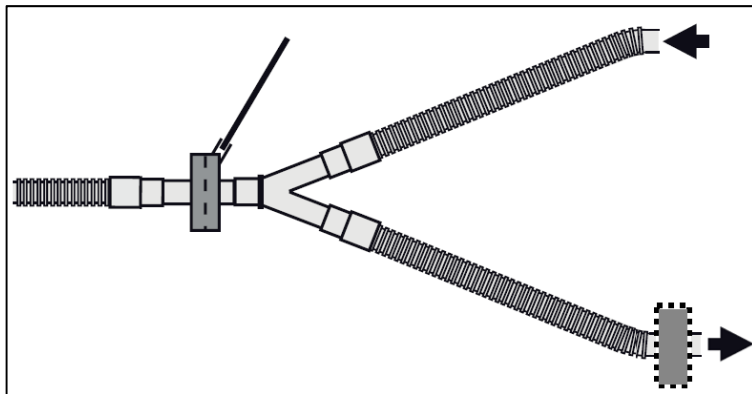


Figure 2

(see figure 2).

Important:

- During ventilation using the above-mentioned setup, the resistance can potentially exceed values demanded by the standard (ISO 80601-2-13:2011). Close monitoring of the respective ventilation and vital parameters is compulsory.
- All Filters used as mentioned above must be mechanical in HEPA Quality (e.g. Dräger SafeStar 80 HEPA (MP01785) and need to be exchanged daily and after each patient.
- For types and part numbers of recommended disposable products, please see the Dräger Accessories Catalogue.

Reprocessing recommendations:

Reprocessing of products, components and surfaces potentially contaminated can be achieved by following the standard procedures described in the Instruction for Use (IfU) and the usage of suitable disinfectants with at least limited virucidal effectiveness. The following recommendations for anesthesia devices contaminated with SARS-CoV-2 are based on general guidelines and practice for infectious diseases. For further details please refer to the newest 'list of surface disinfectants' in the Instructions for Use of your device and/or contact your local sales organization.

Due to

- the so far uncertain infection risk, and
- missing definitive data on its susceptibility to reprocessing measures,

we recommend for the time being the following enhanced procedure as an additional precaution:

C. Essential measures

- C1. Follow the occupational safety and reprocessing guidelines of the hospital and the local/national health authorities.
- C2. Remove all disposable device components which are in contact with the patient's breathing gas:
 - the breathing circuit (hoses),
 - HME/ breathing system filters,
 - sample line and the water trap,
 - endotracheal suction accessories, tubes and filters
 - dispose off all of these safely
- C3. Regarding breathing system reprocessing (including valves & flow sensors), please proceed as described in the Instructions for Use.
- C4. Regarding suction system, please refer to the Instruction for use.
- C5. Clean and disinfect thoroughly with a suitable disinfectant (concentration and exposure time according to manufacturer's instructions) all accessible surfaces of the anaesthesia device, other devices and reusable components.
- C6. Allow to air dry

D. Optional measures following C, if devices were used without a Breathing System Filter (BSF). This part should be in line with the general hospital guideline for all medical devices in the patient vicinity. Prerequisite: All steps described in section C (essential measures) were performed.

- D7. Wrap the anaesthesia device, the other devices and reusable components completely with a plastic cover and store them safely for a specified time (e.g. 21 or 28 days) at room temperature or higher. Make sure all devices are switched off using the main switch to avoid deep discharge of batteries.
- D8. Remove plastic cover and dispose off safely
- D9. Clean and wipe disinfect thoroughly with a suitable disinfectant (concentration and exposure time according to manufacturer's instructions) all accessible surfaces of the anaesthesia device, other devices and reusable components
- D9 Allow to air dry
- D10. Device can be released for reuse.

General Remark: Based on the individual situation, the hospital management responsible for infection control and epidemiology has the task to decide on the required measures. The measures described above are intended for devices used in the recommended manner. Devices used without a Breathing System Filter (BSF) have to be managed in each individual case in consultation with the competent authority. In justified cases of doubt we recommend the safe disposal of contaminated devices and reusable accessories.

If you have further questions, please do not hesitate to ask your local Dräger office for assistance.

Dräger can also provide personal protective equipment (PPE) for healthcare professionals.

With best regards,

Stefan Thal



System Product Manager
Infection Prevention & Control
Business Unit IT & Systeme
Medical Division
Drägerwerk AG & Co. KGaA

Dr. Arne Martensen



Consultant for hygiene / environmental medicine
Specialist for microbiology, virology and
epidemiology of infectious diseases
on behalf of Hygienisches Versorgungszentrum
Hamburg (for specialist knowledge)